RoboSep™-S Software Version 1.5.3 Installation Procedure

This procedure is for upgrading RoboSep™-S (Catalog #21000) software from version 1.5.2 to 1.5.3.

Items Required

- USB keyboard and mouse
- USB flash drive containing the **Update_RoboSep-S_v153** installer

Note: If the installer is contained in a zip file, it will need to be extracted (right click the zip file then select "Extract All") prior to starting the installation procedure.

Installation Procedure

1. If the instrument is on and the RoboSep™-S software is open, close the software on the Homepage by selecting the **[Maintenance]** icon and then **[Exit to Desktop]**.
2. Connect the USB keyboard and mouse to the RoboSep™-S instrument.
3. Insert the USB flash drive containing the **Update_RoboSep-S_v153** installer file into the remaining USB port on the front of the RoboSep™-S instrument.
4. Using Windows File Explorer, navigate to the installer file saved on the USB flash drive. Right click "**Update_RoboSep-S_v153**" and select "**Run as administrator**" to execute the file in admin mode.

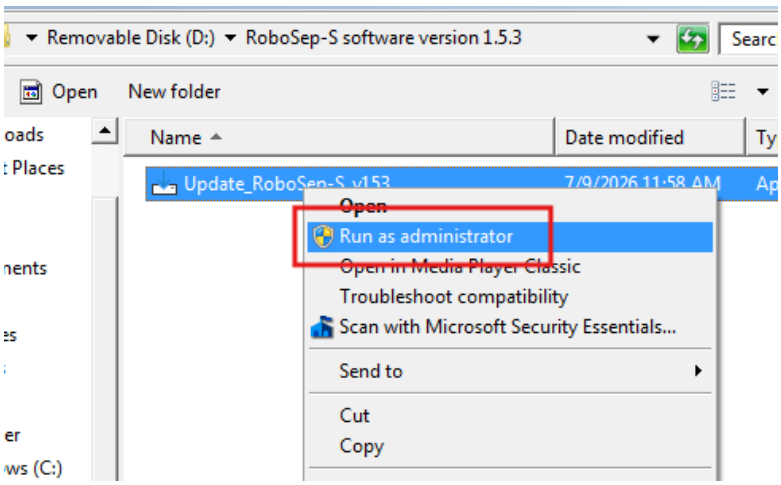

5. Click “**Yes**” to continue installing the update.

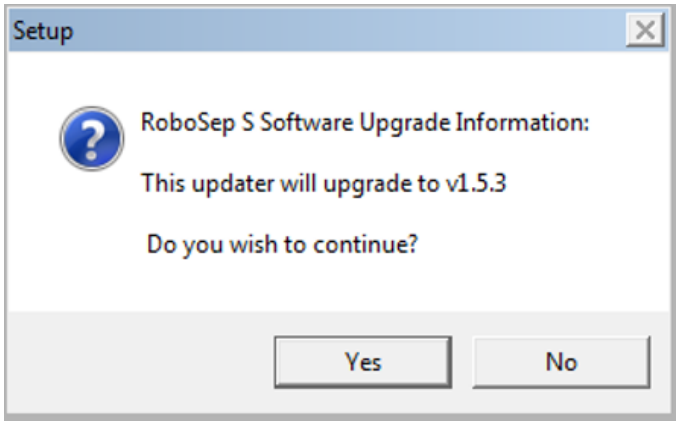

6. Click “**Install**”.

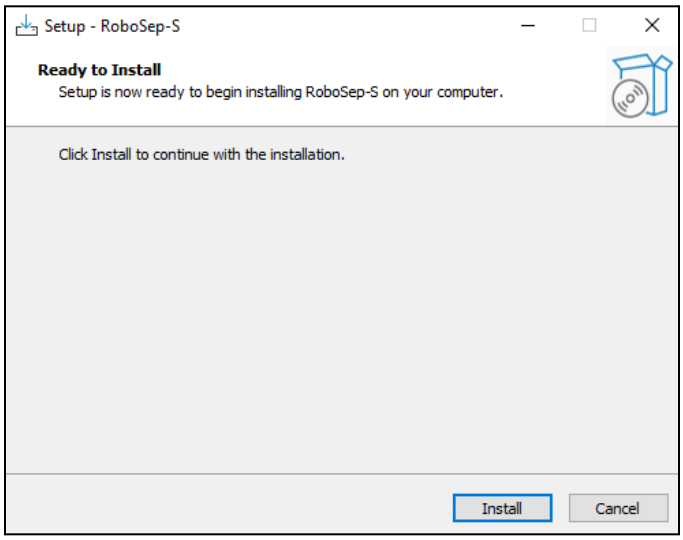

7. For Pump Configuration, leave as “**Manual Configuration**” and click “**Next**”.

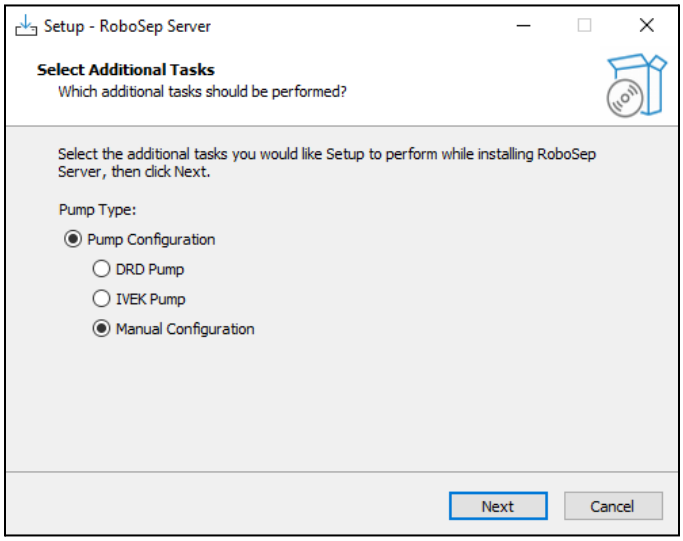

8. At the “**Ready to Install**” page, select “**Install**”.

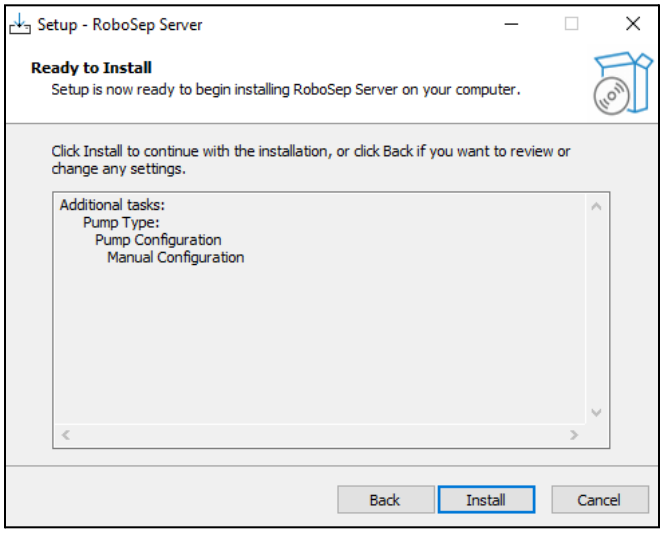

9. Upon completion, a "**DllRegisterServer in RotateTrans.ax succeeded.**" message will appear. Dismiss by clicking "**OK**".

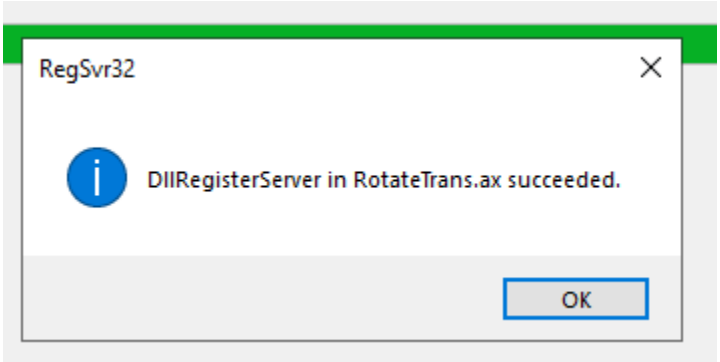

10. Installation of the **RoboSep Server** is now complete. Select "**Finish**".

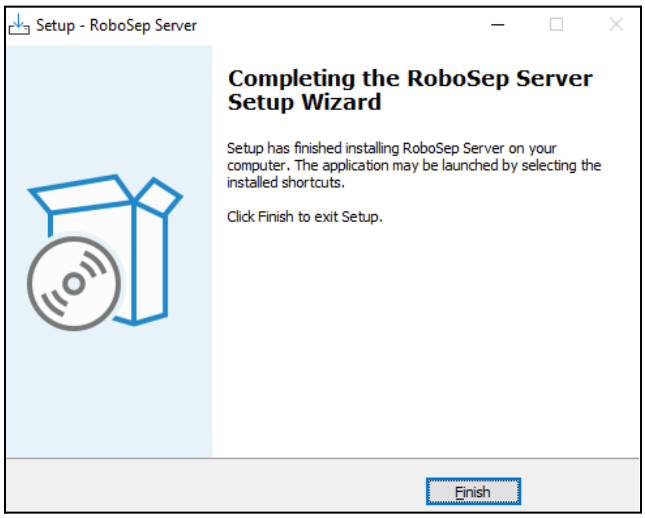

11. Select "**Next**" to proceed with the software installation.

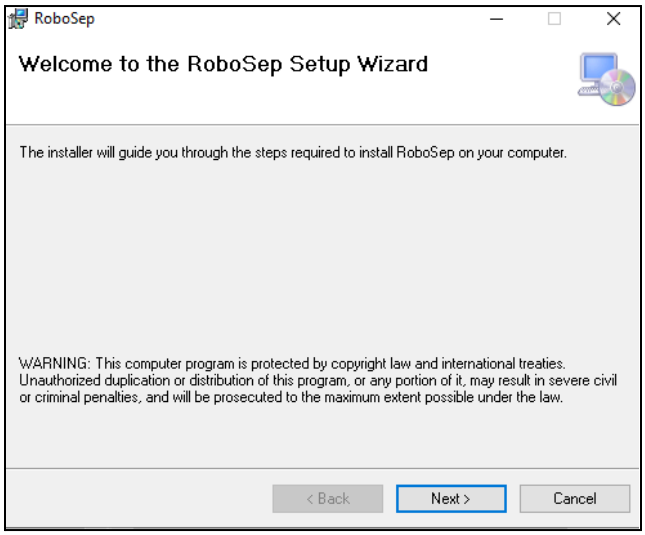

12. Select “**Everyone**” for the installation folder and then click “**Next**”.

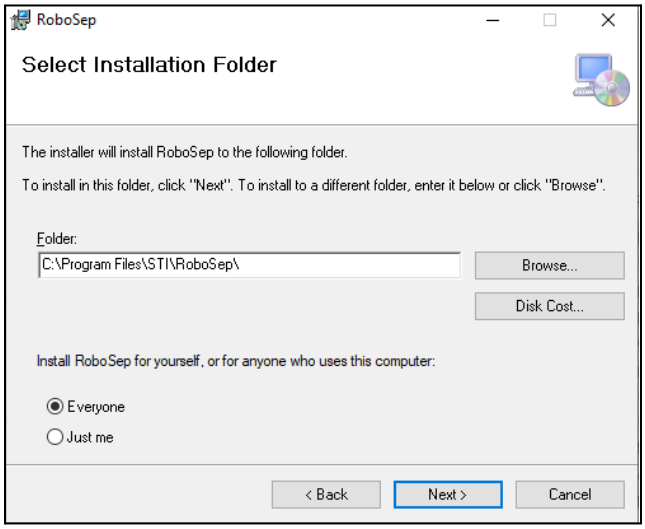

13. In the **“Confirm Installation**” window, select “**Next**” to complete the installation.

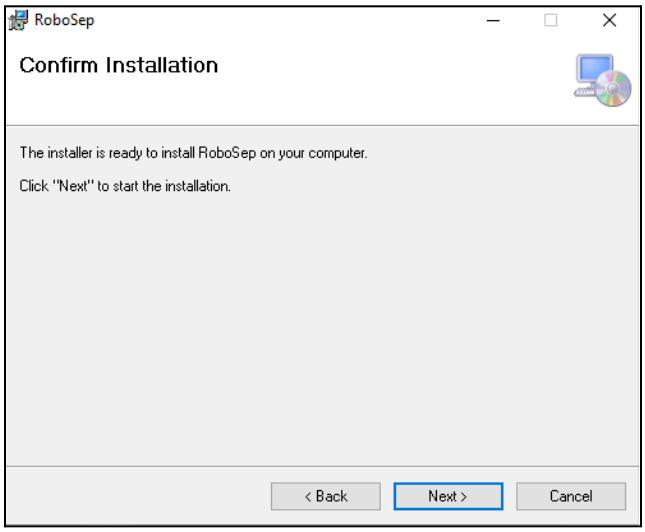

14. Installation of the **RoboSep** application is complete. Click “**Close**”.

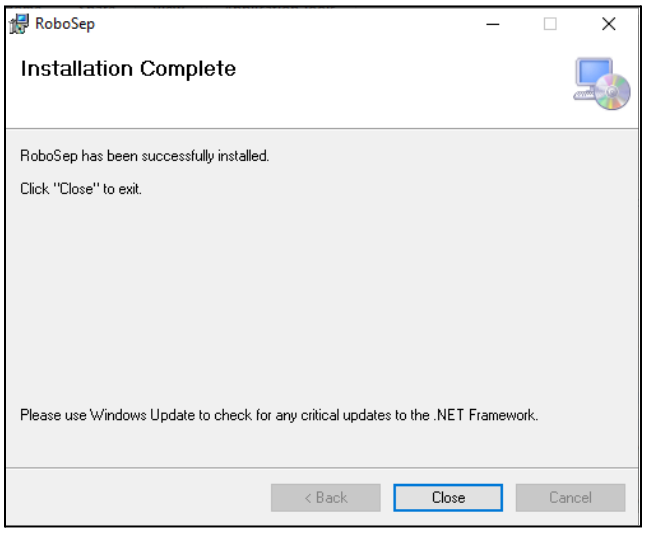

15. Install the **RoboSepService** application. Click “**Next**”.

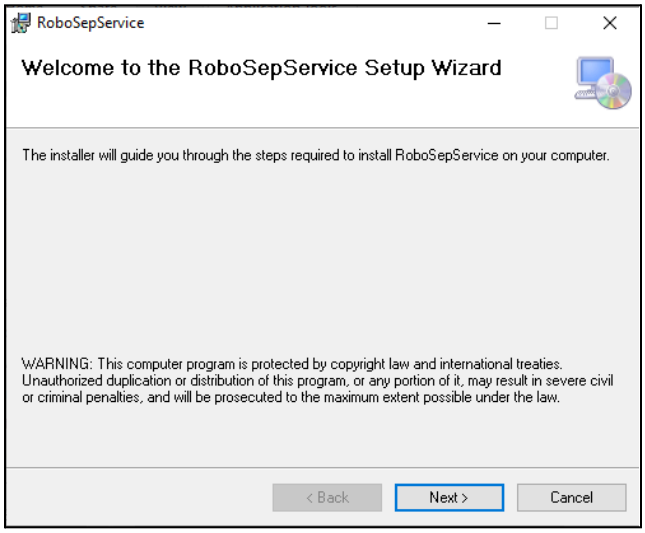

16. Select “**Just me**” for the **RoboSepService** installation folder and click “**Next**”.

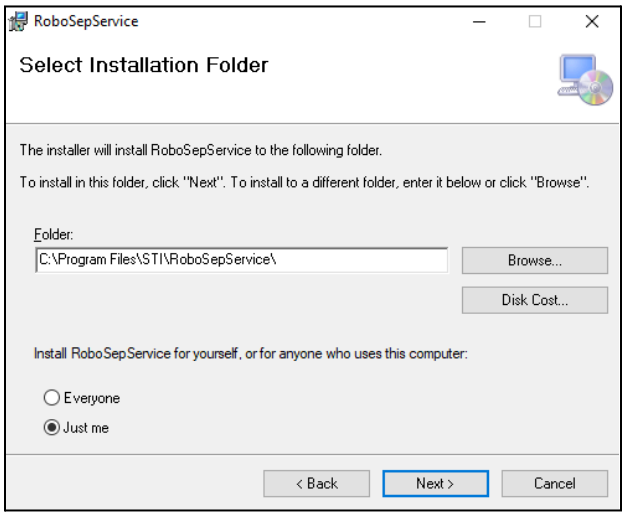

17. In the **“Confirm Installation**” window, select “**Next**”.

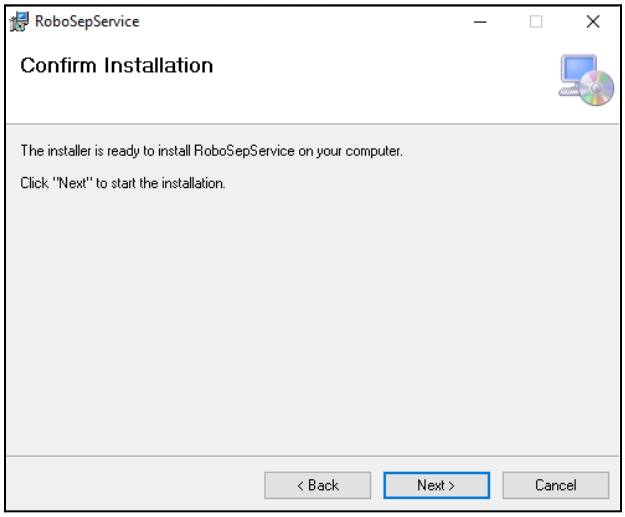

18. Installation of the **RoboSepService** application is now complete. Click “**Close**”.

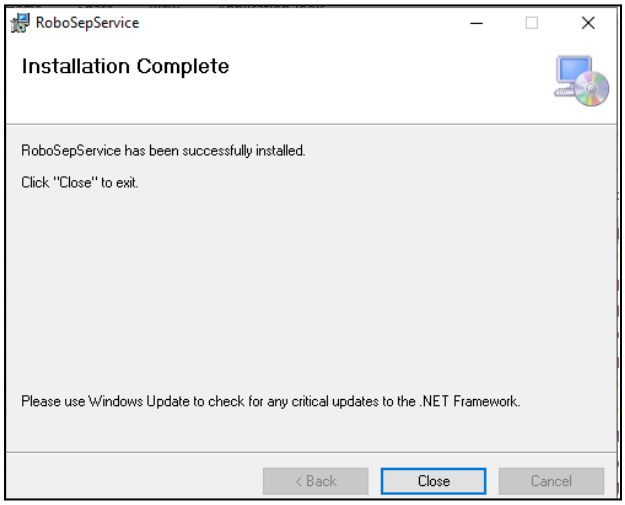

19. All RoboSep™-S applications have now been installed. Select “**No, I will restart the computer later**” when prompted to restart the computer.

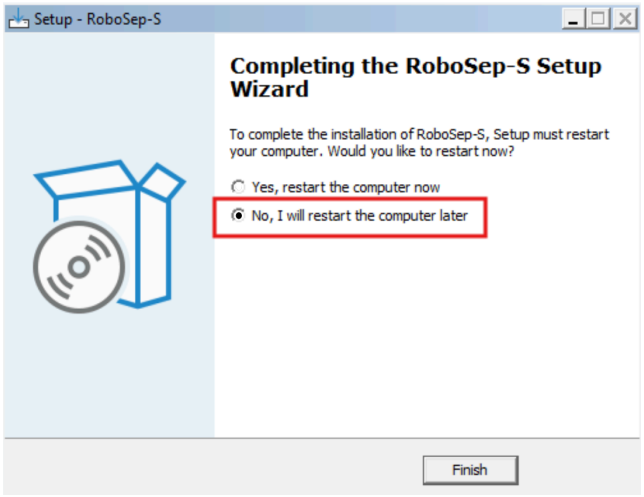

20. Remove the USB flash drive from the RoboSep™-S instrument.

21. Restart the RoboSep™-S device via the Windows menu (press the Windows key on keyboard).

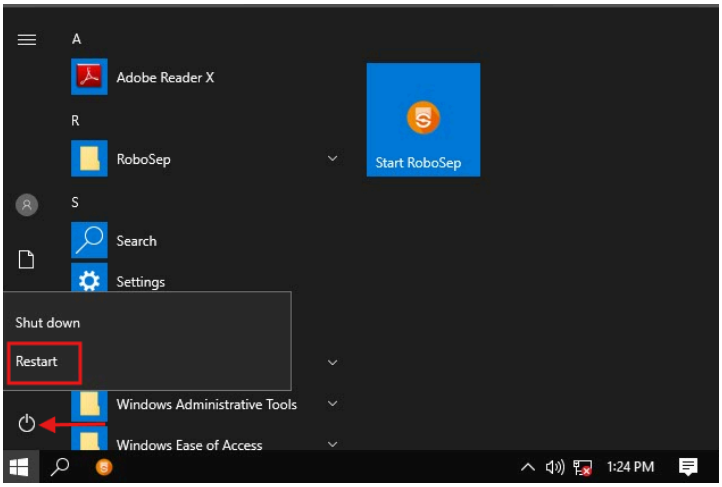
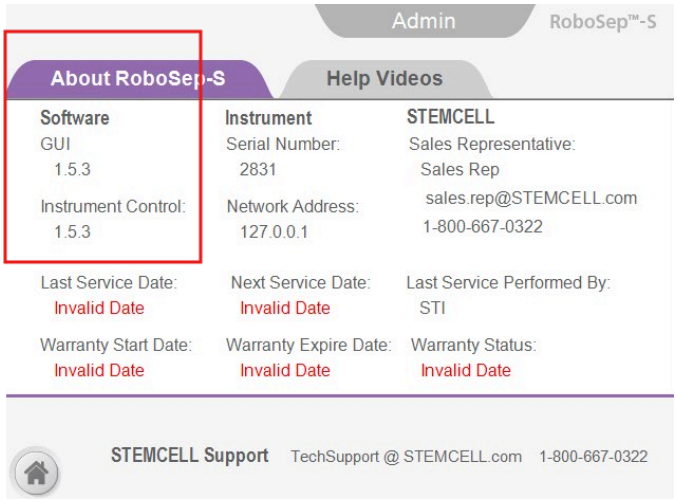
22. Allow RoboSep™-S to restart and for the software to fully load. The RoboSep™ Software will automatically relaunch upon startup. Confirm RoboSep™-S Software Version 1.5.3 was installed by clicking the [**Help**] icon on the Homepage and checking the software version displayed on the "**About RoboSep-S**" page.