

# EasySep™ Human CD4 Positive Selection Kit II



Scientists Helping Scientists™ | [WWW.STEMCELL.COM](http://WWW.STEMCELL.COM)

TOLL FREE PHONE 1 800 667 0322 • PHONE +1 604 877 0713

[INFO@STEMCELL.COM](mailto:INFO@STEMCELL.COM) • [TECHSUPPORT@STEMCELL.COM](mailto:TECHSUPPORT@STEMCELL.COM)

FOR GLOBAL CONTACT DETAILS VISIT OUR WEBSITE

Catalog #100-0693

Positive Selection

Document #10000011776 | Version 01

## Description

Isolate highly purified CD4+ cells from fresh leukapheresis samples by immunomagnetic positive selection.

- Fast and easy-to-use
- Up to 98% purity with high recovery
- No columns required

This kit targets CD4+ cells for positive selection with antibodies recognizing the CD4 surface marker. Desired cells are labeled with antibodies and magnetic particles and separated without columns using an EasySep™ magnet. Unwanted cells are simply pipetted off, while desired cells remain in the flask. Isolated cells are immediately available for downstream applications, such as flow cytometry, culture, or DNA/RNA extraction.

NOTE: This is the Product Information Sheet (PIS) for isolating CD4+ cells using the Easy 250 EasySep™ Magnet (Catalog #100-0821). If using other magnets, refer to the applicable PIS, available at [www.stemcell.com](http://www.stemcell.com) or contact us to request a copy.

## Component Descriptions

COMPONENT NAME	COMPONENT #	QUANTITY	STORAGE	SHELF LIFE	FORMAT
EasySep™ Human CD4 Positive Selection Cocktail II	300-0296	1 x 5 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A combination of monoclonal antibodies in PBS with 10% HPCD and 0.09% rHA.
EasySep™ Dextran RapidSpheres™ 50103	50103	2 x 1 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A suspension of magnetic particles in water.

HPCD - 2-hydroxypropyl-β-cyclodextrin; PBS - phosphate-buffered saline; rHA - recombinant human albumin

Components may be shipped at room temperature (15 - 25°C) but should be stored as indicated above.

## Sample Preparation

For available fresh samples, see [www.stemcell.com/primarycells](http://www.stemcell.com/primarycells).

NOTE: Working with fresh lysed leukapheresis samples is recommended for optimal performance. Alternatively, washed leukapheresis samples may be used (see below) for faster sample processing, but a reduction in performance may be observed.

### LYSED LEUKAPHERESIS

1. Add an equal volume of Ammonium Chloride Solution (Catalog #07800) to the Leukopak (e.g. Human Peripheral Blood Leukopak, Fresh, Catalog #70500\*).  
NOTE: If working with large volumes (> 150 mL), concentrate the Leukopak first by centrifuging at 300 x g for 10 minutes. Remove the supernatant and resuspend the cells in 1/10th of the original Leukopak volume with the recommended medium (e.g. for 300 mL of cells, resuspend in 30 mL of the recommended medium and add 30 mL of Ammonium Chloride Solution). For small volumes (≤ 150 mL), add Ammonium Chloride Solution directly to the Leukopak.
2. Incubate on ice for 15 minutes.
3. Centrifuge at 300 x g for 10 minutes at room temperature (15 - 25°C). Remove the supernatant.
4. Wash the cells by topping up the tube with the recommended medium. Centrifuge the cells at 120 x g for 10 minutes at room temperature with the brake off. Carefully remove the supernatant.
5. Repeat step 4 one or more times until most of the platelets have been removed (indicated by a clear supernatant).
6. Resuspend the cells at 1 x 10<sup>8</sup> cells/mL in the recommended medium.

\* Some primary cell products are available only in select regions. Contact us at [techsupport@stemcell.com](mailto:techsupport@stemcell.com) for further information.

### WASHED LEUKAPHERESIS

Wash the fresh peripheral blood leukapheresis sample (e.g. Human Peripheral Blood Leukopak, Fresh) by adding an equivalent volume of the recommended medium or PBS containing 2% fetal bovine serum (FBS). Centrifuge at 300 x g for 10 minutes at room temperature (15 - 25°C). If platelet removal is necessary, centrifuge at 120 x g for 10 minutes with the brake off. Remove the supernatant and resuspend the cells at 1 x 10<sup>8</sup> cells/mL in the recommended medium.


## Recommended Medium

EasySep™ Buffer (Catalog #20144), RoboSep™ Buffer (Catalog #20104), or PBS containing 2% FBS and 1 mM EDTA. Medium should be free of Ca++ and Mg++.

## Directions for Use – Manual EasySep™ Protocols

See pages 1 and 2 for Sample Preparation and Recommended Medium. Refer to Table 1 for detailed instructions regarding the EasySep™ procedure.

**Table 1. EasySep™ Human CD4 Positive Selection Kit II Protocol**

STEP	INSTRUCTIONS	Easy 250 EasySep™ Magnet (Catalog #100-0821)	
1	Prepare sample at the indicated cell concentration within the volume range.	1 x 10 <sup>8</sup> cells/mL 20 - 100 mL	
	Add sample to required flask.	T-75 cm <sup>2</sup> cell culture flask (i.e. Corning Catalog #353135)	
2	Add Selection Cocktail to sample. NOTE: Do not vortex cocktail.	50 µL/mL of sample	
	Mix and incubate (see Notes and Tips).	RT for 3 minutes	
3	Vortex RapidSpheres™. NOTE: Particles should appear evenly dispersed.	30 seconds	
4	Add RapidSpheres™ to sample.	12 µL/mL of sample	
	Mix and incubate (see Notes and Tips).	RT for 3 minutes	
5	Place the flask (without cap) into the magnet and incubate.	RT for 10 minutes	
6	Carefully pipette (do not pour) off the supernatant (see Notes and Tips). Remove the flask, containing the isolated cells, from the magnet.	Discard supernatant	
7	Add recommended medium to top up sample to the indicated volume. Be sure to resuspend the cells from the side of the flask. Mix by gently pipetting up and down 2 - 3 times.	<ul style="list-style-type: none"> <li>Top up to 5X the original sample volume for samples ≥ 20 - 50 mL</li> <li>Top up to 250 mL for samples &gt; 50 - 100 mL</li> </ul>	
	Place the flask (without cap) into the magnet and incubate.	RT for 10 minutes	
8	Carefully pipette (do not pour) off the supernatant. Remove the flask, containing the isolated cells, from the magnet.	Discard supernatant	
9	Repeat steps as indicated. Be sure to resuspend the cells from the side of the flask.	Steps 7 and 8 (total of 3 x 10-minute separations)	
10	Resuspend cells in desired medium. Be sure to resuspend the cells from the side of the flask. Carefully pipette (do not pour) the cell suspension into a new tube or centrifuge bottle.	Use a new tube or centrifuge bottle*	
11	Centrifuge sample; carefully aspirate and discard supernatant.	Centrifuge at 300 x g for 10 minutes at RT with low brake	
	Resuspend to the desired cell concentration using recommended medium.	Isolated cells are ready for use	

RT - room temperature (15 - 25°C)

\* e.g. 50 mL (30 x 115 mm) conical tube (Catalog #38010) or 225 mL centrifuge bottle (Corning Catalog #352075)

## Notes and Tips

- After addition of Cocktail and RapidSpheres™, mix the sample with a 25 mL or 50 mL serological pipette (e.g. Catalog #38005/38006).  
NOTE: Mixing can also be performed by rotating or gently agitating the flask. Cap the flask first to prevent spillage.
- To remove the supernatant, gently sweep the pipette back and forth along the midline of the T-75 cm<sup>2</sup> flask while aspirating. Avoid touching the sides of the flask. Switch to a 10 mL or smaller serological pipette to collect the residual supernatant.

### ASSESSING PURITY


The EasySep™ Human CD4 Positive Selection Cocktail II uses an anti-CD4 antibody clone that to our knowledge may block other anti-CD4 antibody clones used to assess purity by flow cytometry. For purity assessment of CD4+ cells by flow cytometry, use the following fluorochrome-conjugated antibody clone:

- Anti-Human CD4 Antibody, Clone OKT4 (Catalog #60016)

One of the following methods can also be used:

- Use alternative markers such as fluorochrome-conjugated Anti-Human CD3 Antibody, Clone UCHT1 (Catalog #60011) and Anti-Human CD8a Antibody, Clone RPA-T8 (Catalog #60022). CD4+ T cells will be CD3+CD8-.
- Use a fluorochrome-conjugated secondary antibody, such as Goat Anti-Mouse IgG (H+L) Antibody, Polyclonal (Catalog #60138).

## Data

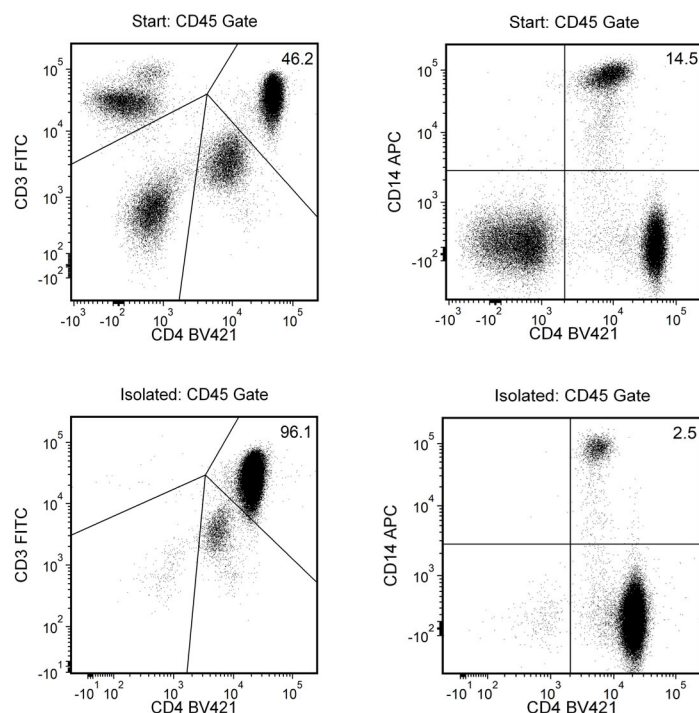

Starting with washed or lysed leukapheresis samples, the CD4+ T cell content (CD4+CD45+) of the isolated fraction is typically  $96.4 \pm 1.6\%$  (gated on CD45, mean  $\pm$  SD for the Easy 250 EasySep™ Magnet). In the above example, the purities of the start and final isolated fractions are 46.2% and 96.1%, respectively. In the above example, the CD14+CD4mid/lo monocyte population decreases from 14.5% in the start fraction to 2.5% in the final isolated fraction.

PRODUCTS ARE FOR RESEARCH USE ONLY AND NOT INTENDED FOR HUMAN OR ANIMAL DIAGNOSTIC OR THERAPEUTIC USES UNLESS OTHERWISE STATED. FOR ADDITIONAL INFORMATION ON QUALITY AT STEMCELL, REFER TO [WWW.STEMCELL.COM/COMPLIANCE](http://WWW.STEMCELL.COM/COMPLIANCE).

Copyright © 2025 by STEMCELL Technologies Inc. All rights reserved including graphics and images. STEMCELL Technologies & Design, STEMCELL Shield Design, Scientists Helping Scientists, EasySep, and RapidSpheres are trademarks of STEMCELL Technologies Canada Inc. Corning is a registered trademark of Corning Incorporated. All other trademarks are the property of their respective holders. While STEMCELL has made all reasonable efforts to ensure that the information provided by STEMCELL and its suppliers is correct, it makes no warranties or representations as to the accuracy or completeness of such information.