



EasySep™ Direct Human Total Lymphocyte Isolation Kit

Negative Selection
Catalog #19655

For processing 100 mL whole blood



Scientists Helping Scientists™ | WWW.STEMCELL.COM

TOLL FREE PHONE 1 800 667 0322 • PHONE +1 604 877 0713
INFO@STEMCELL.COM • TECHSUPPORT@STEMCELL.COM
FOR GLOBAL CONTACT DETAILS VISIT OUR WEBSITE

Document #28080 | Version 1_4_1

Description

Isolate highly purified lymphocytes directly from human whole blood, buffy coat, or spleen by immunomagnetic negative selection.

The benefits of this kit include:

- > 99.9% RBC depletion without the need for density gradient centrifugation, sedimentation, or lysis
- Fast, easy-to-use and column-free
- Up to 96% purity of isolated cells
- Isolated cells are untouched

This kit targets non-lymphocytes for removal with antibodies recognizing specific surface markers. Unwanted cells are labeled with antibodies and EasySep™ Direct RapidSpheres™, and separated using an EasySep™ magnet. Desired cells are simply collected into a new tube and are immediately available for downstream applications such as flow cytometry, culture, or DNA/RNA extraction.

Component Descriptions

Components may be shipped at room temperature (15 - 25°C) and should be refrigerated upon receipt. Precipitate may be observed in the cocktail vial but will not affect performance.

EasySep™ Direct Human Total Lymphocyte Isolation Kit (Catalog #19655)

COMPONENT NAME	COMPONENT #	QUANTITY	STORAGE	SHELF LIFE	FORMAT
EasySep™ Direct Human Total Lymphocyte Isolation Cocktail	19655C	2 x 2.5 mL	Store at 2 - 8°C.	Stable until expiry date (EXP) on label.	A combination of monoclonal antibodies in PBS.
EasySep™ Direct RapidSpheres™ 50300	50300	4 x 2.5 mL	Store at 2 - 8°C.	Stable until expiry date (EXP) on label.	A suspension of magnetic particles and monoclonal antibodies in PBS.

PBS - phosphate-buffered saline

EasySep™ Direct Human Total Lymphocyte Isolation Kit for RoboSep™ (Catalog #19655RF)

COMPONENT NAME	COMPONENT #	QUANTITY	STORAGE	SHELF LIFE	FORMAT
EasySep™ Direct Human Total Lymphocyte Isolation Cocktail for RoboSep™	19655CRF	4 x 1.25 mL	Store at 2 - 8°C.	Stable until expiry date (EXP) on label.	A combination of monoclonal antibodies in PBS.
EasySep™ Direct RapidSpheres™ 50301	50301	8 x 1.25 mL	Store at 2 - 8°C.	Stable until expiry date (EXP) on label.	A suspension of magnetic particles and monoclonal antibodies in PBS.

PBS - phosphate-buffered saline

Sample Preparation

PERIPHERAL BLOOD

For optimal RBC depletion, collect blood using heparin or acid citrate dextrose (ACD) as an anticoagulant.

For best recovery, use unprocessed human whole blood. Recovery of the desired isolated cells decreases with samples that are older than 24 hours.

The volume of blood that can be processed depends on the EasySep™ magnet used for the isolation procedure. Blood samples must be placed in the required tube to properly fit into the appropriate EasySep™ magnet (see Tables 1 and 2).

BUFFY COAT

1. Add an equal volume of recommended medium to whole blood.
2. Centrifuge at 800 x g for 10 minutes at room temperature (15 - 25°C) with the brake off.
3. Remove the concentrated leukocyte band (this is the buffy coat), plus a small portion of the plasma and concentrated red blood cells (RBCs). The target is to concentrate the leukocytes approximately 5-fold while maintaining the same hematocrit (e.g. collect 2 mL of buffy coat when starting with 10 mL of whole blood).
4. Transfer buffy coat to the required tube.

SPLEEN

Disrupt spleen in PBS or Hanks' Balanced Salt Solution (HBSS) containing 2% fetal bovine serum (FBS). Remove aggregates and debris by passing the cell suspension through a pre-wetted 100 µm mesh nylon strainer. Rinse the strainer with PBS or HBSS containing 2% FBS. Centrifuge at 300 x g for 10 minutes and resuspend at 1 - 100 x 10⁶ cells/mL in recommended medium.



Recommended Medium

EasySep™ Buffer (Catalog #20144), RoboSep™ Buffer (Catalog #20104), D-PBS (Without Ca⁺⁺ and Mg⁺⁺; Catalog #37350), or PBS containing 2% FBS and 1 mM EDTA. Medium should be free of Ca⁺⁺ and Mg⁺⁺.

Directions for Use – Manual EasySep™ Protocols

See pages 1 and 2 for Sample Preparation and Recommended Medium. Refer to Tables 1 and 2 for detailed instructions regarding the EasySep™ procedure for each magnet.

Table 1. EasySep™ Direct Human Total Lymphocyte Isolation Kit Protocol for WHOLE BLOOD, BUFFY COAT, or SPLEEN




		EASYSEP™ MAGNETS	
STEP	INSTRUCTIONS	 EasySep™ (Catalog #18000)	 “The Big Easy”™ (Catalog #18001)
1	Collect sample within the volume range.	0.5 - 1.5 mL	1.5 - 7 mL
	Add whole blood sample to required tube.	5 mL (12 x 75 mm) polystyrene round-bottom tube (e.g. Catalog #38007)	14 mL (17 x 95 mm) polystyrene round-bottom tube (e.g. Catalog #38008)
2	Vortex RapidSpheres™. NOTE: Particles should appear evenly dispersed.	30 seconds	30 seconds
3	Add Isolation Cocktail to sample.	50 µL/mL of sample	50 µL/mL of sample
4	Add RapidSpheres™ to sample.	50 µL/mL of sample	50 µL/mL of sample
5	Mix and incubate.	RT for 5 minutes	RT for 5 minutes
6	Add recommended medium to top up the sample to the indicated volume. Mix by gently pipetting up and down 2 - 3 times.	Top up to 2.5 mL	<ul style="list-style-type: none"> • Top up to double the volume for samples ≤ 5 mL • Top up to 10 mL for samples > 5 mL
7	Place the tube (without lid) into the magnet and incubate.	RT for 5 minutes	RT for 5 minutes
8	Pick up the magnet, and in one continuous motion invert the magnet and tube, pouring the enriched cell suspension* into a new tube.	Use a new 5 mL tube	Use a new 14 mL tube
9	Add RapidSpheres™ to the new tube containing the enriched cells.	Use same volume as in step 4	Use same volume as in step 4
	Mix and incubate.	RT for 5 minutes	RT for 5 minutes
10	Remove the tube from the magnet and place the tube from step 9 (without lid) into the magnet and incubate for a second separation.	RT for 5 minutes	RT for 5 minutes
11	Pick up the magnet, and in one continuous motion invert the magnet and tube,** pouring the enriched cell suspension into a new tube.	Isolated cells are ready for use	Use a new 14 mL tube
12	Remove the tube from the magnet and place the new tube (without lid) into the magnet and incubate for a third separation.	---	RT for 5 minutes
13	Pick up the magnet, and in one continuous motion invert the magnet and tube,** pouring the enriched cell suspension into a new tube.	---	Isolated cells are ready for use

RT; room temperature (15 - 25°C)

* Following the first magnetic separation the collected cells may contain a significant amount of RBCs and may look similar to the original unprocessed human whole blood sample.

** To minimize RBC contamination in the isolated cells, pour off the sample along a clean area of the tube (i.e. the opposite side to where the sample was poured in).

Table 2. EasySep™ Direct Human Total Lymphocyte Isolation Kit Protocol for WHOLE BLOOD, BUFFY COAT, or SPLEEN

STEP	INSTRUCTIONS	EASYSEP™ MAGNETS		
		 EasyEights™ (Catalog #18103)		 Easy 50 (Catalog #18002)
		5 mL tube	14 mL tube	
1	Collect sample within the volume range.	0.5 - 1.5 mL	1.5 - 7 mL	7 - 30 mL
	Add whole blood sample to required tube.	5 mL (12 x 75 mm) polystyrene round-bottom tube (e.g. Catalog #38007)	14 mL (17 x 95 mm) polystyrene round-bottom tube (e.g. Catalog #38008)	50 mL (30 x 115 mm) conical tube (e.g. Catalog #38010)
2	Vortex RapidSpheres™. NOTE: Particles should appear evenly dispersed.	30 seconds	30 seconds	30 seconds
3	Add Isolation Cocktail to sample.	50 µL/mL of sample	50 µL/mL of sample	50 µL/mL of sample
4	Add RapidSpheres™ to sample.	50 µL/mL of sample	50 µL/mL of sample	50 µL/mL of sample
5	Mix and incubate.	RT for 5 minutes	RT for 5 minutes	RT for 5 minutes
6	Add recommended medium to top up the sample to the indicated volume. Mix by gently pipetting up and down 2 - 3 times.	Top up to 2.5 mL	<ul style="list-style-type: none"> Top up to double the volume for samples ≤ 5 mL Top up to 10 mL for samples > 5 mL 	<ul style="list-style-type: none"> Top up to double the volume for samples ≤ 25 mL Top up to 50 mL for samples > 25 mL
7	Place the tube (without lid) into the magnet and incubate.	RT for 5 minutes	RT for 5 minutes	RT for 10 minutes
8	Carefully pipette*** (do not pour) the enriched cell suspension into a new tube. NOTE: Collect the entire clear fraction from top to bottom. For optimal recovery, also collect a small volume of RBCs (up to 10% of the starting sample volume).	Use a new 5 mL tube	Use a new 14 mL tube	Use a new 50 mL tube
9	Add RapidSpheres™ to the new tube containing the enriched cells.	Use same volume as in step 4	Use same volume as in step 4	Use same volume as in step 4
	Mix and incubate.	RT for 5 minutes	RT for 5 minutes	RT for 5 minutes
10	Remove the tube from the magnet and place the tube from step 9 (without lid) into the magnet and incubate for a second separation.	RT for 5 minutes	RT for 5 minutes	RT for 5 minutes
11	Carefully pipette*** (do not pour) the enriched cell suspension into a new tube. NOTE: Collect only the clear fraction.	Use a new 5 mL tube	Use a new 14 mL tube	Use a new 50 mL tube
12	Remove the tube from the magnet and place the new tube (without lid) containing the enriched cells into the magnet and incubate for a third separation.	RT for 5 minutes	RT for 5 minutes	RT for 5 minutes
13	Carefully pipette*** (do not pour) the enriched cell suspension into a new tube. NOTE: Collect only the clear fraction.	Isolated cells are ready for use	Isolated cells are ready for use	Isolated cells are ready for use

RT; room temperature (15 - 25°C)

*** Collect the entire enriched cell suspension, all at once, into a single pipette (e.g. for EasyEights™ 5 mL tube use a 2 mL serological pipette [Catalog #38002]; for EasyEights™ 14 mL tube use a 10 mL serological pipette [Catalog #38004]).

Directions for Use – Fully Automated RoboSep™ Protocol

See pages 1 and 2 for Sample Preparation and Recommended Medium. Refer to Table 3 for detailed instructions regarding the RoboSep™ procedure.

Table 3. RoboSep™ Direct Human Total Lymphocyte Isolation Kit Protocol for WHOLE BLOOD, BUFFY COAT, or SPLEEN

STEP	INSTRUCTIONS	RoboSep™ (Catalog #20000 and #21000)
1	Prepare sample within the volume range.	For blood or spleen: 0.5 - 6 mL For buffy coat: 2 - 5 mL 14 mL (17 x 95 mm) polystyrene round-bottom tube (e.g. Catalog #38008)
	Add sample to required tube.	
2	Select protocol. [§]	Human Total Lymphocyte Negative Isolation from Whole Blood 19655 [§] Human Total Lymphocyte Negative Isolation from Buffy Coat 19655
3	Vortex RapidSpheres™. NOTE: Particles should appear evenly dispersed.	30 seconds
4	Load the carousel.	Follow on-screen prompts
	Start the protocol.	Press the green "Run" button
5	Unload the carousel when the run is complete.	Isolated cells are ready for use

§ Use this protocol if working with spleen.

Notes and Tips

REMOVAL OF RESIDUAL RBCs IN THE ISOLATED CELLS

Typically, further RBC depletion is not required following cell isolation. If residual RBCs are visible in the isolated cell pellet following centrifugation after the end of the protocol, resuspend in a small volume (0.2 - 2.5 mL) of recommended medium or desired culture medium and place in a smaller EasySep™ magnet for an additional 5-minute separation. Collect the supernatant; the isolated cells are ready for use in downstream applications. Residual RBCs may also be lysed using Ammonium Chloride Solution (Catalog #07800).

ASSESSING PURITY

For purity assessment of total lymphocytes by flow cytometry use the following fluorochrome-conjugated antibody clones:


- Anti-Human CD3 Antibody, Clone UCHT1 (Catalog #60011), and
- Anti-Human CD19 Antibody, Clone HIB19 (Catalog #60005), and
- Anti-Human CD56 (NCAM) Antibody, Clone HCD56 (Catalog #60021; not shown), and
- Anti-Human CD45 Antibody, Clone HI30 (Catalog #60018)

Lymphocytes are either CD3+, CD3-CD19+, or CD3-CD56+.

NOTE: It is recommended to assess purity on CD45+ cells to exclude debris, platelets, and RBCs. Include a viability dye if necessary (e.g. Propidium Iodide [Catalog #75002]; 7-AAD [7-Aminoactinomycin D; Catalog #75001]).

Data

Starting with human whole blood from normal healthy donors, the typical total lymphocyte (CD19+ and CD3+) content of the non-lysed final isolated fraction is 96.7 ± 1.5% (gated on CD45) or 95.8 ± 2.2% (not gated on CD45).

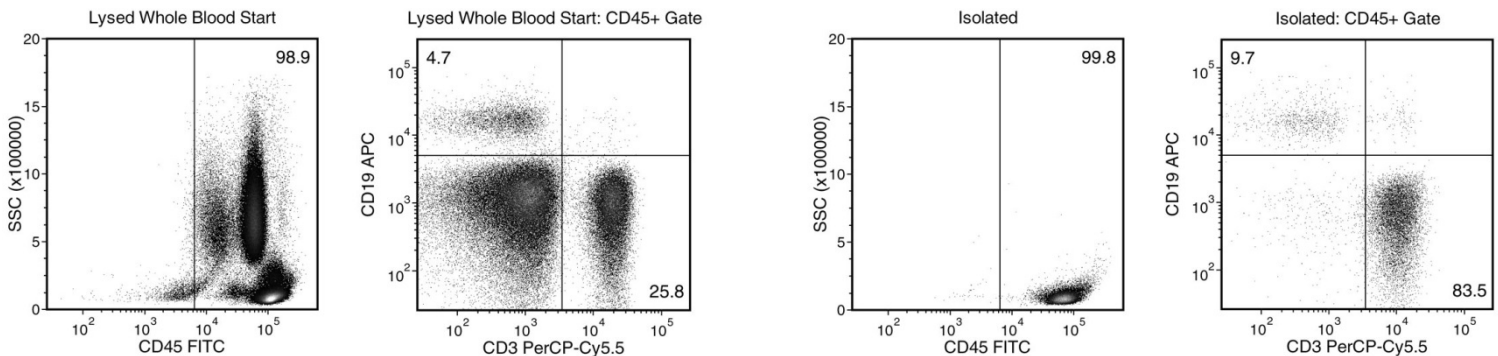

In the above example, the total lymphocyte (CD19+ and CD3+) content of the lysed whole blood start sample and non-lysed final isolated fraction is 30.5% and 93.2% (gated on CD45), respectively, or 30.2% and 93.0% (not gated on CD45), respectively. The starting frequency of total lymphocytes in the non-lysed whole blood start sample above is 0.055% (data not shown).

STEMCELL TECHNOLOGIES INC.'S QUALITY MANAGEMENT SYSTEM IS CERTIFIED TO ISO 13485. PRODUCTS ARE FOR RESEARCH USE ONLY AND NOT INTENDED FOR HUMAN OR ANIMAL DIAGNOSTIC OR THERAPEUTIC USES UNLESS OTHERWISE STATED.

Copyright © 2018 by STEMCELL Technologies Inc. All rights reserved including graphics and images. STEMCELL Technologies & Design, STEMCELL Shield Design, Scientists Helping Scientists, EasyEights, EasySep, RapidSpheres, and RoboSep are trademarks of STEMCELL Technologies Canada Inc. All other trademarks are the property of their respective holders. While STEMCELL has made all reasonable efforts to ensure that the information provided by STEMCELL and its suppliers is correct, it makes no warranties or representations as to the accuracy or completeness of such information.