



## EasySep™ Human Plasmacytoid DC Enrichment Kit

Negative Selection  
Catalog #19062

For processing  $2 \times 10^9$  cells



Scientists Helping Scientists™ | [WWW.STEMCELL.COM](http://WWW.STEMCELL.COM)

TOLL FREE PHONE 1 800 667 0322 • PHONE +1 604 877 0713  
INFO@STEMCELL.COM • TECHSUPPORT@STEMCELL.COM  
FOR GLOBAL CONTACT DETAILS VISIT OUR WEBSITE

Document #29149 | Version 3\_0\_0

## Description

Isolate untouched and highly purified plasmacytoid dendritic cells (pDCs) from fresh human peripheral blood mononuclear cells (PBMCs) by immunomagnetic negative selection.

- Fast, easy-to-use and column-free
- Up to 97% purity
- Untouched, viable cells

This kit targets non-pDCs including myeloid dendritic cells (mDCs) for removal with antibodies recognizing specific cell surface markers. Unwanted cells are labeled with antibodies and magnetic particles, and separated without columns using an EasySep™ magnet. Desired cells are simply poured off into a new tube. Isolated cells are immediately available for downstream applications such as flow cytometry, culture, or DNA/RNA extraction.

## Component Descriptions

COMPONENT NAME	COMPONENT #	QUANTITY	STORAGE	SHELF LIFE	FORMAT
EasySep™ Human Plasmacytoid DC Enrichment Cocktail Component A	19062C.1	2 x 1 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A combination of monoclonal antibodies in PBS.
EasySep™ Human DC Enrichment Cocktail Component B	19060C	2 x 1 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A combination of monoclonal antibodies in PBS.
EasySep™ D Magnetic Particles ‡	19250	8 x 1 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A suspension of magnetic particles in TBS.
Anti-Human CD32 (Fc gamma RII) Blocker, for negative selection	14551C	2 x 0.8 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A combination of monoclonal antibodies in PBS.

PBS - phosphate-buffered saline; TBS - TRIS-buffered saline

‡ When using the Easy 50 EasySep™ Magnet, contact us at [techsupport@stemcell.com](mailto:techsupport@stemcell.com) to request an additional vial of EasySep™ D Magnetic Particles.

Components may be shipped at room temperature (15 - 25°C) but should be stored as indicated above.

## Sample Preparation

For available fresh and frozen samples, see [www.stemcell.com/primarycells](http://www.stemcell.com/primarycells).

### PERIPHERAL BLOOD

Prepare a PBMC suspension from whole peripheral blood by centrifugation over a density gradient medium (e.g. Lymphoprep™, Catalog #07801). For more rapid PBMC preparation, use the SepMate™ RUO (Catalog #86450/86415) or SepMate™ IVD\* (Catalog #85450/85415) cell isolation tube.

NOTE: Use of fresh whole blood is strongly recommended. Using day-old blood will result in reduced pDC purities and recoveries.

After preparation, resuspend cells at  $5 \times 10^7$  cells/mL in recommended medium.

\* SepMate™ IVD is only available in select regions where it is registered as an In Vitro Diagnostic (IVD) device for the isolation of mononuclear cells (MNCs) from whole blood or bone marrow by density gradient centrifugation. In all other regions SepMate™ is available for research use only (RUO).



## Recommended Medium

EasySep™ Buffer (Catalog #20144), RoboSep™ Buffer (Catalog #20104), or PBS containing 2% fetal bovine serum (FBS) and 1 mM EDTA. Medium should be free of Ca<sup>++</sup> and Mg<sup>++</sup>.

**Directions for Use – Manual EasySep™ Protocols**

See page 1 for Sample Preparation and Recommended Medium. Refer to Tables 1 and 2 for detailed instructions regarding the EasySep™ procedure for each magnet.

**Table 1. EasySep™ Human Plasmacytoid DC Enrichment Kit Protocol**


		EASYSEP™ MAGNETS	
STEP	INSTRUCTIONS	 <b>EasySep™</b> (Catalog #18000)	<b>“The Big Easy”</b> (Catalog #18001) 
1	Prepare sample at the indicated cell concentration within the volume range.	5 x 10 <sup>7</sup> cells/mL 0.25 - 2 mL	5 x 10 <sup>7</sup> cells/mL 0.5 - 8 mL
	Add sample to required tube.	5 mL (12 x 75 mm) polystyrene round-bottom tube (e.g. Catalog #38007)	14 mL (17 x 95 mm) polystyrene round-bottom tube (e.g. Catalog #38008)
2	Add FcR Blocker to sample.‡	30 µL/mL of sample	30 µL/mL of sample
3	Add Plasmacytoid DC Enrichment Cocktail Component A to sample.	50 µL/mL of sample	50 µL/mL of sample
4	Add DC Enrichment Cocktail Component B to sample.	50 µL/mL of sample	50 µL/mL of sample
	Mix and incubate.	RT for 30 minutes	RT for 30 minutes
5	Vortex Magnetic Particles. NOTE: Particles should appear evenly dispersed.	30 seconds	30 seconds
6	Add Magnetic Particles to sample.	200 µL/mL of sample	200 µL/mL of sample
	Mix and incubate.	RT for 10 minutes	RT for 10 minutes
7	Add recommended medium to top up the sample to the indicated volume. Mix by gently pipetting up and down 2 - 3 times.	Top up to 2.5 mL	<ul style="list-style-type: none"> <li>• Top up to 3.5 mL for samples ≤ 2 mL</li> <li>• Top up to 6.5 mL for samples &gt; 2 - 5 mL</li> <li>• Top up to 10 mL for samples &gt; 5 mL</li> </ul>
	Place the tube (without lid) into the magnet and incubate.	RT for 5 minutes	RT for 5 minutes
8	Pick up the magnet, and in one continuous motion invert the magnet and tube,* pouring the enriched cell suspension into a new tube.	Use a new 5 mL tube	Use a new 14 mL tube
9	Remove the tube from the magnet and place the new tube (without lid) into the magnet and incubate for a second separation.	RT for 5 minutes	RT for 5 minutes
10	Pick up the magnet, and in one continuous motion invert the magnet and tube,* pouring the enriched cell suspension into a new tube.	Isolated cells are ready for use	Isolated cells are ready for use

RT - room temperature (15 - 25°C)

‡ Addition of Anti-Human CD32 (Fc gamma RII) Blocker may prevent downstream attempts at cross-linking CD32 molecules to trigger signaling through these receptors. The FcR Blocker may be omitted if necessary.

\* Leave the magnet and tube inverted for 2 - 3 seconds, then return upright. Do not shake or blot off any drops that may remain hanging from the mouth of the tube.

**Table 2. EasySep™ Human Plasmacytoid DC Enrichment Kit Protocol**

		EASYSEP™ MAGNETS	
STEP	INSTRUCTIONS	Easy 50 (Catalog #18002)	
1	Prepare sample at the indicated cell concentration within the volume range.	5 x 10 <sup>7</sup> cells/mL Up to 35 mL	
	Add sample to required tube.	50 mL (30 x 115 mm) conical tube (e.g. Catalog #38010)	
2	Add FcR Blocker to sample.‡	30 µL/mL of sample	
3	Add Plasmacytoid DC Enrichment Cocktail Component A to sample.	50 µL/mL of sample	
4	Add DC Enrichment Cocktail Component B to sample.	50 µL/mL of sample	
	Mix and incubate.	RT for 30 minutes	
5	Vortex Magnetic Particles. NOTE: Particles should appear evenly dispersed.	30 seconds	
6	Add Magnetic Particles to sample.	250 µL/mL of sample	
	Mix and incubate.	RT for 10 minutes	
7	Add recommended medium to top up sample to the indicated volume. Mix by gently pipetting up and down 2 - 3 times.	<ul style="list-style-type: none"> <li>• Top up to 10 mL for samples &lt; 5 mL</li> <li>• Top up to 20 mL for samples ≥ 5 - 10 mL</li> <li>• Top up to 30 mL for samples &gt; 10 - 15 mL</li> <li>• Top up to 40 mL for samples &gt; 15 - 20 mL</li> <li>• Top up to 50 mL for samples &gt; 20</li> </ul>	
	Place the tube (without lid) into the magnet and incubate.	RT for 5 minutes	
8	Carefully pipette** (do not pour) the enriched cell suspension into a new tube.	Use a new 50 mL tube	
9	Remove the tube from the magnet and place the new tube (without lid) into the magnet and incubate for a second separation.	RT for 5 minutes	
10	Carefully pipette** (do not pour) the enriched cell suspension into a new tube.	Isolated cells are ready for use	

RT - room temperature (15 - 25°C)

‡ Addition of Anti-Human CD32 (Fc gamma RII) Blocker may prevent downstream attempts at cross-linking CD32 molecules to trigger signaling through these receptors. The FcR Blocker may be omitted if necessary.

\*\* Collect the entire supernatant, all at once, into a single pipette.

**Directions for Use – Fully Automated RoboSep™ Protocol**

See page 1 for Sample Preparation and Recommended Medium. Refer to Table 3 for detailed instructions regarding the RoboSep™ procedure.

**Table 3. RoboSep™ Human Plasmacytoid DC Enrichment Kit Protocol**

STEP	INSTRUCTIONS	RoboSep™ (Catalog #20000 and #21000)
1	Prepare sample at the indicated cell concentration within the volume range.	5 x 10 <sup>7</sup> cells/mL 0.5 - 8 mL
	Add sample to required tube.	14 mL (17 x 95 mm) polystyrene round-bottom tube (e.g. Catalog #38008)
2	Add FcR Blocker to sample.‡	30 µL/mL of sample
3	Add DC Enrichment Cocktail Component B to sample.	50 µL/mL of sample
3	Select protocol.	<ul style="list-style-type: none"> <li>Human pDC Enrichment 19062-small volume (0.5 - 2.0 mL)</li> <li>Human pDC Enrichment 19062-large volume (2.1 - 5.0 mL)</li> <li>Human pDC Enrichment 19062-mega volume (5.1 - 8.0 mL)</li> </ul>
4	Vortex Magnetic Particles. NOTE: Particles should appear evenly dispersed.	30 seconds
5	Load the carousel.	Follow on-screen prompts NOTE: This protocol requires loading <b>two</b> vials of EasySep™ D Magnetic Particles onto the carousel for a single run; one in the ▲ (triangle) slot and one in the ● (circle) slot.
	Start the protocol.	Press the green "Run" button
6	Unload the carousel when the run is complete.	Isolated cells are ready for use

‡ Addition of Anti-Human CD32 (Fc gamma RII) Blocker may prevent downstream attempts at cross-linking CD32 molecules to trigger signaling through these receptors. The FcR Blocker may be omitted if necessary.


**Notes and Tips**

**ASSESSING PURITY**

pDCs are described as Lineage (CD3, CD14, CD16, CD19, CD20, CD34, CD56)-negative, HLA-DR positive, and CD304 (BDCA-4)-positive. For purity assessment of pDCs by flow cytometry use the following fluorochrome-conjugated antibodies:

- Anti-Human CD3 Antibody, Clone UCHT1 (Catalog #60011), and
- Anti-Human CD14 Antibody, Clone M5E2 (Catalog #60004), and
- Anti-Human CD16 Antibody, Clone 3G8 (Catalog #60041), and
- Anti-Human CD19 Antibody, Clone HIB19 (Catalog #60005), and
- Anti-Human CD20 Antibody, Clone 2H7 (Catalog #60008), and
- Anti-Human CD34 Antibody, Clone 581 (Catalog #60013), and
- Anti-Human CD56 (NCAM) Antibody, Clone HCD56 (Catalog #60021), and
- Anti-Human HLA-DR Antibody, Clone LN3 (Catalog #60164), and
- Anti-human CD304 (BDCA-4) antibody

**Data**

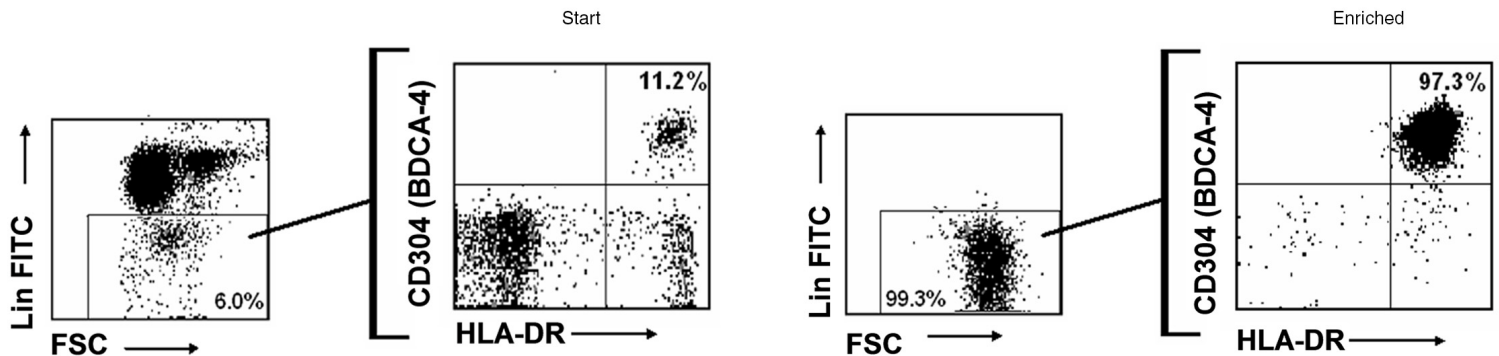

Starting with PBMCs containing 0.2 - 0.9% pDCs, the pDC content (Lin-/HLA-DR+/BDCA-4+) of the enriched fraction typically ranges from 87 - 97%. In the above example, the purities of the start and final enriched fractions are 0.67% and 96.6%, respectively.



Negative Selection

## EasySep™ Human Plasmacytoid DC Enrichment Kit



STEMCELL TECHNOLOGIES INC.'S QUALITY MANAGEMENT SYSTEM IS CERTIFIED TO ISO 13485. PRODUCTS ARE FOR RESEARCH USE ONLY AND NOT INTENDED FOR HUMAN OR ANIMAL DIAGNOSTIC OR THERAPEUTIC USES UNLESS OTHERWISE STATED.

Copyright © 2017 by STEMCELL Technologies Inc. All rights reserved including graphics and images. STEMCELL Technologies & Design, STEMCELL Shield Design and Scientists Helping Scientists, EasySep, RoboSep, and SepMate are trademarks of STEMCELL Technologies Canada Inc. Lymphoprep is a trademark of AXIS-SHIELD. All other trademarks are the property of their respective holders. While STEMCELL has made all reasonable efforts to ensure that the information provided by STEMCELL and its suppliers is correct, it makes no warranties or representations as to the accuracy or completeness of such information.